



MonacoTM

Instruction Manual



Contents

03

Safety
Instructions

05

Technical
Specification

07

User Guide and
Operating Instructions

11

Working
Environment

13

Recycling
Policy

15

Intellectual
Property

17

Maintenance
and Servicing

This Instruction Manual is frequently
updated to ensure safe use of your product.

Visit **seatingmatters.com** where you can
find a free copy of the most up to date version.



Safety Instructions Monaco

All instructions must be read and understood before the product may be used.



Terminologies

Patient

The person sitting in the chair.

User

Competent person with responsibility for the persons sitting in the chair as well as the suitability of the equipment for the Patient. The User is responsible for checking the chair for faults during the course of its use.


Assembly, Installation, Warnings & Hazards

- ① This chair should be fully assembled, all fixings secured and the chair checked for safety by a competent person before use.
- ② The User must ensure that the product is in good condition before use (check all nuts and bolts are fastened, fabric in good condition etc). If there are any problems, these must be reported to your Seating Matters provider and corrected before the chair is put into use.
- ③ Keep all body parts away from the mechanisms under the chair. Repairs and maintenance should only be carried out by fully trained technicians.
- ④ Exercise care in using the release lever for the reclining mechanisms and adjustments to avoid injury.
- ⑤ Pressure ulcer or pressure injury reduction is not a guarantee with this equipment. The User must ensure that the Patient has a period out of the chair after prolonged sitting to raise tissue oxygenation levels. Although the chair offers pressure management, the body tissue still needs time to recover. In many places, local or national guidelines recommend a maximum of 2 hours sitting at any one time. You must also observe Patient specific recommendations and guidelines as set by their health professional with regard to the use of tilt and recline for appropriate pressure management.
- ⑥ The product must be used on a level, plain, hard surface with the brakes engaged to avoid it moving during use and to ensure stability. When the chair is not in transit, all the braking castors on the product must be engaged to prevent risk of injury when being used.
- ⑦ The product may not be left in an outdoor environment. More information on fabrics and their environment can be found later in this manual.
- ⑧ A competent person, trained in the use of the chair, should make adjustments and set it up according to the User requirements and Patient dimensions before the Patient sits in the chair. Where possible, adjustments should be made when the Patient is not in the chair to avoid injury to the User and Patient.
- ⑨ Ensure there is more than one competent person there when making adjustments to ensure they are correct and safe for the Patient.
- ⑩ If in doubt as to any the adjustments, feel free to contact Seating Matters direct at **technical@seatingmatters.com**.
- ⑪ Under no circumstances must the User or Patient stand or sit on the footplate of the chair.
- ⑫ The chair should not be transported in a vehicle while the Patient is seated on the chair.
- ⑬ This product should not be lifted at any time unless by competent persons trained in such manual handling.
- ⑭ When operating the leg rest and recline features on the chair please ensure there is a 450mm gap around the chair to prevent the back or leg rest coming into contact with a wall or any other object.
- ⑮ On powered options, please ensure that your chair is charged daily.

Please call your Seating Matters provider if you have any questions on these points.



Technical Specification Monaco

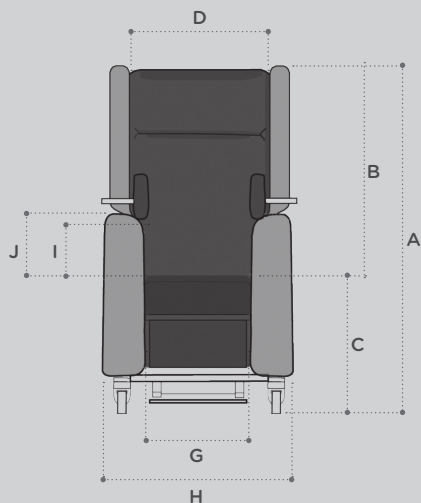

Basic Dimensions

A	Overall height	47.5" / 1205mm
B	Back height	31.5" / 800mm
C	Seat to floor height	14-20" / 350-500mm
D	Inside back width	20" / 505mm
E	Chair length	34" / 870mm
F	Reclined length	43" / 1090mm

Available Seat and Overall Widths

G (Seat Width)	H (Overall Width)
400mm / 16in	26" / 655mm *
450mm / 18in	27" / 690mm *
500mm / 20in	27" / 690mm *
550mm / 22in	29" / 740mm *
600mm / 24in	31" / 790mm *

* Dimension excludes legrest belt. Add 1.5" / 35mm if belt is used.

Arm Height Options*

I	Low	7" / 180mm
J	High	8" / 210mm

Seat Depth Options

K	Min	14-19" / 350-480mm
L	Max	19-22" / 490-550mm

Leg Rest Length

M	16.5" / 420mm
---	---------------

Clearance Height

N	2.4" / 60mm - 5.5" / 140mm
---	----------------------------

Recline and Tilt Angles

ii Back Angle Recline

90° - 130°
40° range

iii Leg Rest Angle

75° - 107°
32° range


iv Angle Adjustable Seat

0° - 20°
20° range

Chair weight unloaded is 10.56 Stone / 57 Kg / 125.6 lb

Chair user weight limit is 25 Stone / 159 Kg / 364 lb

*Please note when adapting cushion thickness arm height will be affected.

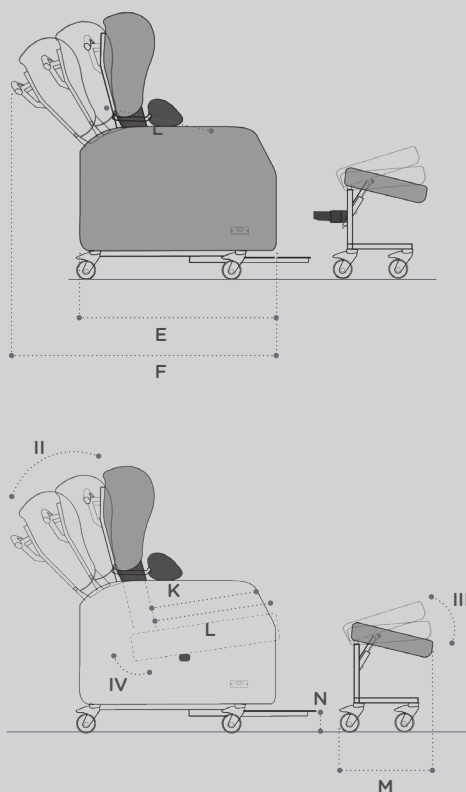




User Guide & Operating Instructions Monaco



Braking Castors

A competent person, trained in the use of the chair, should make adjustments and set it up according to the User requirements and Patient dimensions before the Patient sits in the chair. Ensure there is more than one competent person present when making adjustments to ensure they are correct and safe. Ensure all fixings are secure before allowing the person to sit in the chair, this includes lateral supports, seat adjustment and footplate. Please call your Seating Matters provider if you have any questions on these points. This product should not be lifted at any time unless by competent persons trained in such manual handling.


The **Monaco™** must be used on a plane, hard surface with the brakes engaged to ensure stability and to avoid the device moving undesirably during use. Braking castors, where provided, must be in the braked position while in use (**fig.1**).

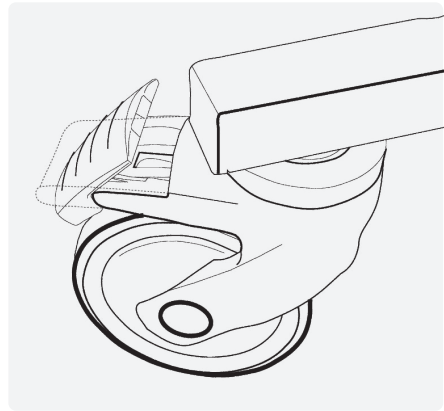

(fig.1)

Back Angle Adjustment

To recline the back of the chair, the user must inform the Patient then stand behind the chair, and with two hands, firmly hold the push handle while closing the release lever (**fig.2**). Move the back of the chair slowly until it is in the required position and allow the release lever to move to its relaxed position before letting go of the push handles.

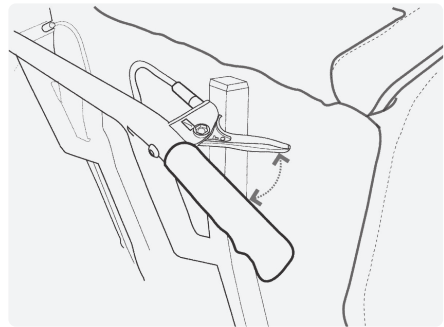

(fig.2)



Back Angle Adjustment

To adjust the angle of the seat on the chair, the User must inform the Patient then stand behind the chair, firmly hold the push handle with your right hand and close the release lever located at the back of the chair (labelled TILT) with your left hand (**fig.3**). While closing the release lever place your foot on the step (labelled STEP) and push down until the seat is at the required angle and allow the release lever to move to its relaxed position before letting go of the push handles.

Please Note: do not change the angle of the seat before informing the patient sitting in the chair.




(fig.3)


Seat Depth Adjustment

To adjust the seat depth on the Monaco™ loosen the two wing knobs (**fig.4 & 5**) positioned under the seat of the chair, move the seat to the desired position and tighten the wing knobs again.

Please Note: Do not attempt to adjust the seat depth while the client is in the chair.

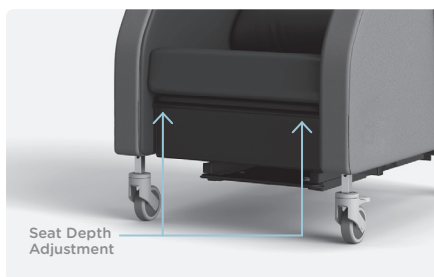

(fig.4)

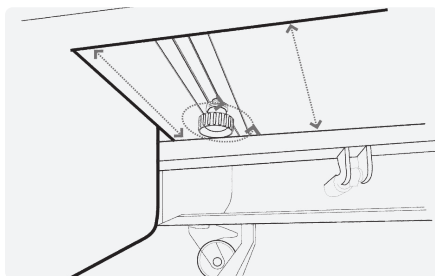

(fig.5)

Seat Height Adjustment

This adjustment is a factory setting. Please contact your Seating Matters provider for further adjustment.

Chair Movement

To move the **Monaco™** around, ensure the brakes are disengaged and push using the push handle on the back. Only a competent person should move this chair. Engage the directional lock castor on the front left of the chair to control the direction of movement and for ease of manoeuvrability.


Seat Cushion

The seat cushion on the **Monaco™** is a waterproof, pressure redistributing, breathable, medium foam cushion providing pressure management and comfort. The seat cushion will have non-slip material on one face and a zip closure on one side.

To fit the seat cushion to the chair, unwrap the cushion from the plastic packaging. Ensure the non-slip material is on the bottom and makes contact with the non-slip material already on the baseboard, with the zip closure at the rear. This is important as the foam's structure facilitates immersion and envelopment of the body prominences **ONLY** when fitted as instructed.

Sliding Footplate

At no point should anyone stand or sit on the sliding footplate. To use the sliding footplate pull it out to the full position and allow the feet to rest on it, ensuring they are placed on top of the sliding footplate. Push the footplate in to its fully retracted position before allowing the Patient to get on or off the chair, exercising care to stay away from the sliding rail. Adjust the footplate by holding the front lip.

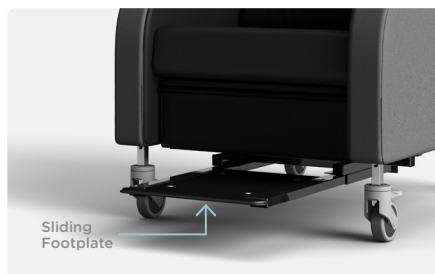

(fig.6)

Stand Transfers

Ensure the sliding footplate is fully retracted before allowing the patient to get on or off the chair exercising care to stay away from the sliding rail. Ensure the braking castors are engaged for stability and safety. The back recline and seat angle must be in a safe position before the Patient can perform the stand transfer. These functions are adjusted manually (see image with back recline and seat angle adjustment levers).



Working Environment



Dartex Multi-stretch is waterproof, stain resistant, flame retardant, multidirectional stretch fabric for pressure management situations – i.e. seat cushion, calf panels, lateral supports and seat back.

Vinyl is non-absorbent, anti-bacterial, flame retardant, strong, durable material for outer arms, outside back etc.

Cleaning and Maintenance of Fabrics

Vinyl

(Arms and outside back) Vinyl is resistant to urine, most household stains, mild acids/alkalis, drinks and beverages as they are not absorbed by the vinyl and can be wiped off without any problem or lasting damage. Some difficult substances such as lipstick, ball point pen ink and food colourings should be cleaned off immediately to avoid permanent staining.

Cleaning

To ensure proper cleaning and longevity of the fabrics, the chairs should be cleaned with warm soapy water followed by a clean water rinse to help retain the attractive appearance and durability. Heavy, ingrained soiling may be removed by scrubbing with a soft brush. Strong detergents, solvent cleaners, polishes or patent chemical cleaners should not be used as they are unnecessary and may cause embrittlement and cracking of the material. Additional Care – special attention should be given to head rest and arm rest areas, as build-up of body oils in these areas will gradually cause the vinyl to harden.

Dartex Multi Stretch Fabric (Patient contact surface)

Properties

This fabric is waterproof, can be wiped clean and has biostatic (anti-mycotic) coatings to provide an impenetrable barrier to virus and bacteria. Superficial dirt may be removed by wiping with a soft cloth moistened with water containing a neutral detergent. More persistent contamination may be treated by wiping with alcohols or turpentine substitute, followed by hot water and detergent.

Routine cleaning and disinfection in situ may be carried out on the coating with hand hot water and a neutral detergent or with a sodium hypochlorite solution (0.1% or 1000 parts per million available chlorine). The material is compatible with the 10,000ppm available chlorine in solution required for the decontamination of blood spills. Excess solution must be removed and the surface thoroughly rinsed and dried prior to reuse or storage. Proprietary disinfectants may be used provided manufacturer's instructions are followed. All cleaning agents, and disinfectants, must be thoroughly rinsed off and the item dried before storage.

Failure to do this may result in damage to the polyurethane coating, react with the chair frame, or negate the biocompatibility results of the fabric. It is essential that articles be thoroughly dried after all cleaning procedures and before storage.



Recycling Policy

Seating Matters are committed to reducing waste and improving our care for the environment. We aimed to construct our chairs with as many recyclable materials as possible that could be repurposed indefinitely.



The WEEE Directive

The WEEE Directive, 2012/19/EC, urges producers of Electrical and Electronic Equipment (EEE) to provide information on how these products can be treated, reused or recycled.

In order to comply with this directive in the European Union, Seating Matters electrical components are marked with a crossed out wheelie bin. This indicates that the electrical components should be treated in accordance with the WEEE regulations after their useful life.

Advice on Recycling

- ① Your Seating Matters product may contain batteries which should not be disposed of in household waste.
- ② Never dispose of the battery in a fire. This may cause an explosion.
- ③ The product may contain substances that could be harmful to the environment.
- ④ Electrical components must be taken to a proper recycling facility.
- ⑤ Your Seating Matters product contains component parts which can be recycled.
- ⑥ We thank you for being environmentally responsible and for making efforts to recycle your Seating Matters product at the end of its' safe and useful life.
- ⑦ Contact your local authority or governmental agency for the regulations that apply in your area.
- ⑧ If you wish to have Seating Matters recycle your product and your behalf, you are welcome to return the product to our company.



Plastic Components

Many of our plastic components are made from polypropylene and can be recycled as long as they are recycled with other polypropylene resin materials. Polypropylene sheets can be recycled with any other materials that have this symbol.



Plastic Trays

Our plastic tray tables are made from Polyethylene Terephthalate Glycol (PETG) which is a sturdy, transparent, easily cleaned material. Like acrylic, PETG is 100% recyclable and can be recycled and repurposed indefinitely. Capable of being sterilized, it's a renowned food-safe material and will help us meet a higher standard towards infection prevention & control. PETG's damage resistance is far higher than that of acrylic & has an impact resistance 30 times that of glass. PETG can be recycled with any other materials that have this symbol.



Safety


The **Monaco™** is CE marked to show conformance to the Medical Devices Directive 93/42/EEC and conforms to BS ISO 7176 at medium hazard.

Regional Variations

The device referred to as a **Monaco™** is a Seating Matters product category and the information included in this document reflects common features of this group of products. In some regions of the world, we supply product design variations of equivalent function and ease-of-use but with alternative specifications or reinforcements.



Intellectual Property

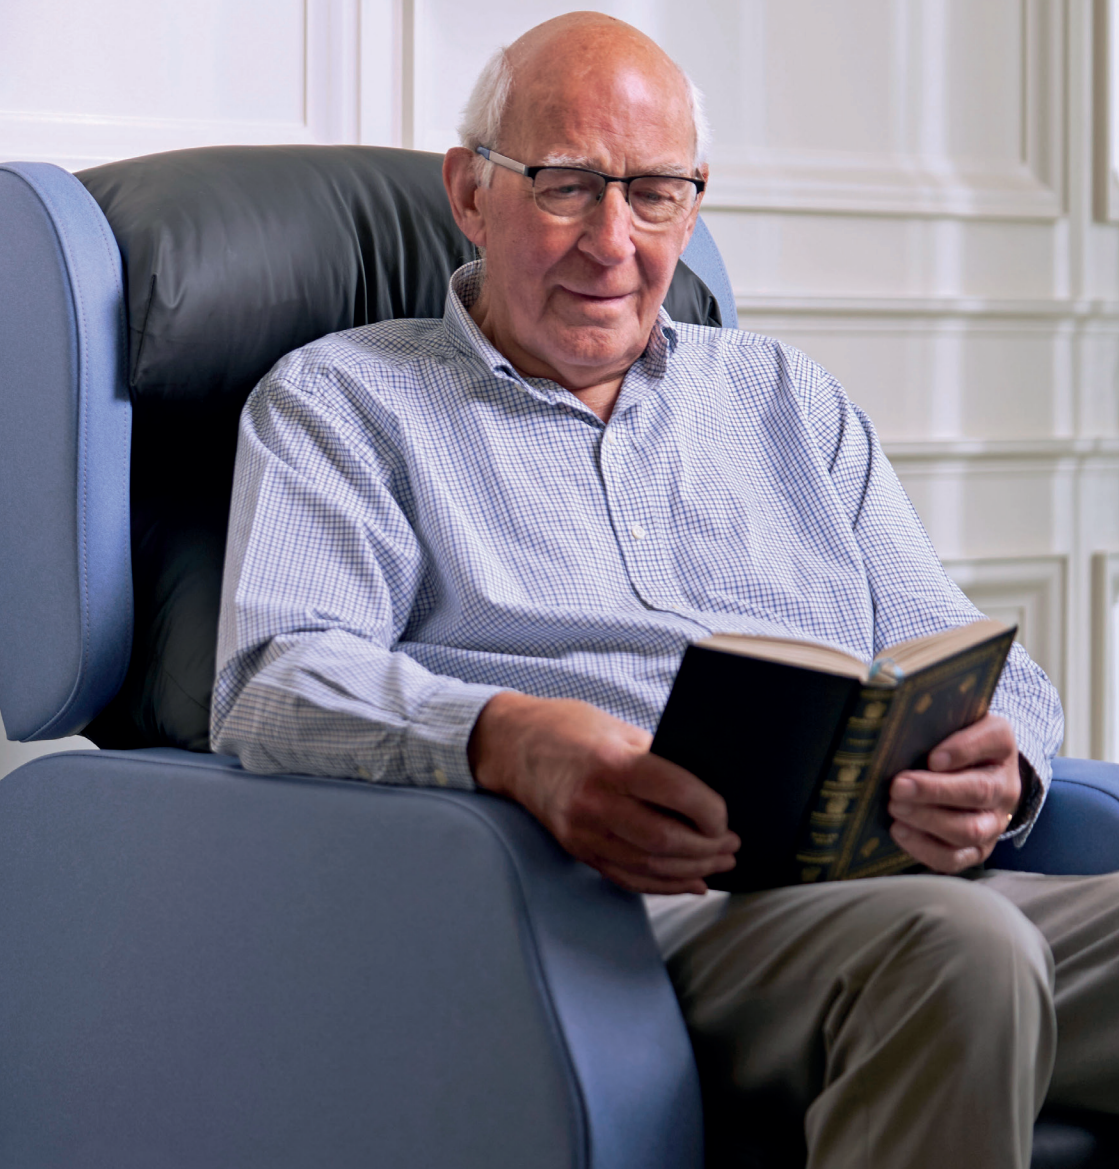

Seating Matters are at the forefront of seating research and design, therefore we take the protection of our intellectual property very seriously and have our designs, patents and trademarks protected in many jurisdictions throughout the world.

The Seating Matters Trademark is registered throughout the European Union and various countries globally.

Patent Pending	No. GB1915470.7
-----------------------	-----------------

US Design Patent	No. 601360S No. D611718 No. 600932 No. D602704S
-------------------------	--

Australian Design Registration	No. 325536 No. 324011 No. 325537 No. 324012
---------------------------------------	--

Community Design Registration	No. 001016364-002 No. 000942180-0004 No. 002428813-0001 No. 001016364-001 No. 012673018
--------------------------------------	---

Canadian Design Registration	No. 130224 No. 128763 No. 130217 No. 128764
-------------------------------------	--

We are here to help

For any questions or queries regarding your Seating Matters chair please contact:
contact@seatingmatters.com



Maintenance & Servicing



Regularly servicing your Seating Matters chair will prevent untimely and inconvenient breakdowns, reduce repair costs and extend the chair's life. Damage to the chair can also cause excess strain for the Patient and User.

Important

Parts can only be changed by service persons trained in Seating Matters products and use only Seating Matters parts. We recommend that your chair is serviced every year by a Seating Matters approved provider for any running repairs and maintenance.

Maintenance

Carry out the following regular checks to ensure the operation and safety of the chair. If you are in any doubt about the functioning of your chair contact your Seating Matters approved provider immediately.

Daily

- ① Check that the castors are not damaged.
- ② Check that the castors turn freely.
- ③ Make sure that the castor forks run free and are not bent.
- ④ Check all fabrics for damage or contamination and replace where necessary.
- ⑤ See cleaning and maintenance of fabrics section in manual for cleaning instructions.

Weekly

- ① Check the castors fittings for hair and dirt etc. which could restrict the castor movement.
- ② Pick out any such material with tweezers or take the spindle out, clean it and then replace it.
- ③ If it is still not free (one continuous turn without it sticking) contact your Seating Matters approved provider for replacement.

Monthly

Castors

Make sure the top of the castor housing is parallel with the floor. Any variation will cause restricted movement. If it is damaged contact your Seating Matters approved provider for replacement.

Mechanisms

Check all tilting mechanisms are working smoothly.

Check that all nuts and bolts are present and secure.

Please Note: If nuts or bolts need attention, contact your Seating Matters approved provider immediately and do not use the chair until it has been serviced.

Leg Rest

Check that all leg rests are easily removed/ swung-away and replaced or repositioned easily. Ensure that parts lock in place securely. If parts are not locking try lubricating. If the problem still remains contact your Seating Matters approved provider.

Frame

Check the visible parts of the frame for cracks, splits, large dents or other damage. If you find any of these things **DO NOT USE**. Contact your Seating Matters approved provider immediately.



Just ask the Patient...







We are here to help

For any questions or queries regarding your Seating Matters chair.

Please contact: **contact@seatingmatters.com**



**Australia**

9/256 New Line Road
Dural
NSW 2158
Australia
T: +61 1300 001 050
australia@seatingmatters.com

Canada

269 Maplegrove Road
Colborne, ON
Canada
K0K 1S0
T: +1 (905) 507 9007
canada@seatingmatters.com

USA

300 International Dr
Suite 100, Buffalo
New York, USA
NY 14221
T: +1 (905) 507 9007
usa@seatingmatters.com

UK & Europe

1st Floor
239 High Street, Kensington
London, UK
W8 6SN
T: +44 (0) 20 3982 2900
london@seatingmatters.com

N. Ireland & ROI

131 Carnamuff Road
Limavady
Northern Ireland
BT49 9JG
T: +44 (0) 28 777 666 24
contact@seatingmatters.com

